

Enzyme immunoassaying apparatus  
[Sample assaying apparatus]


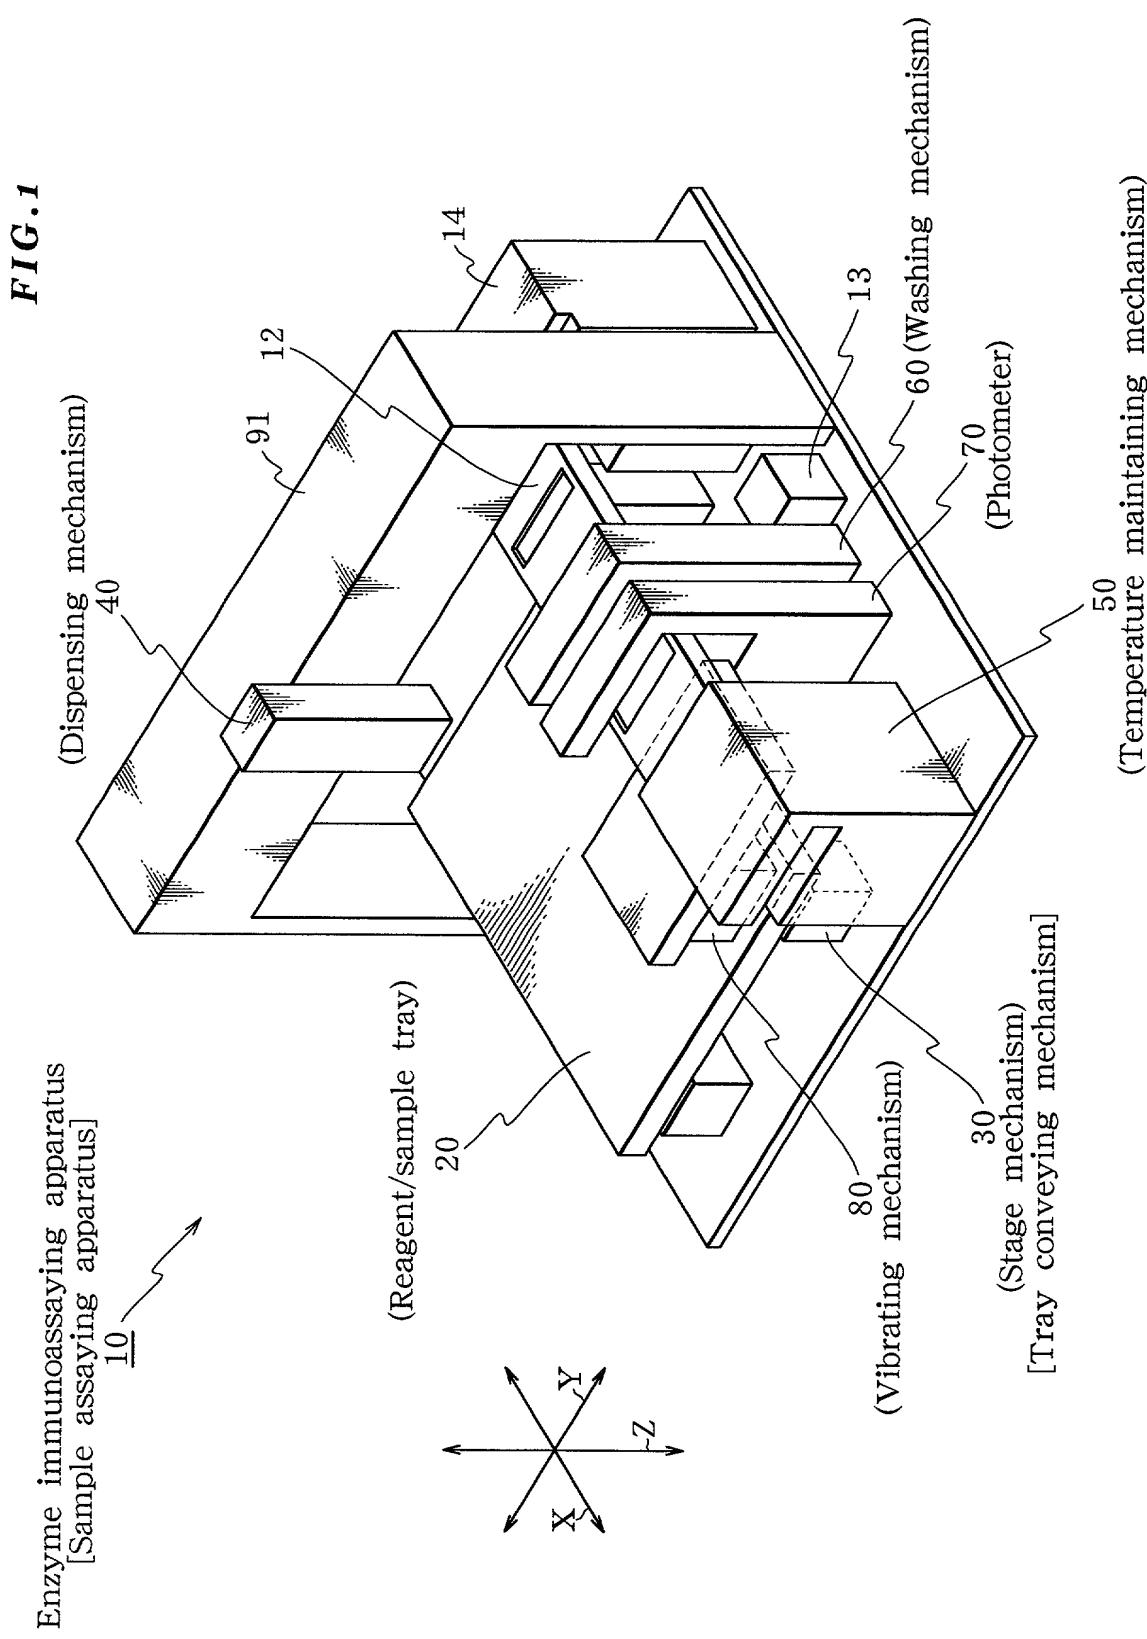


FIG. 2

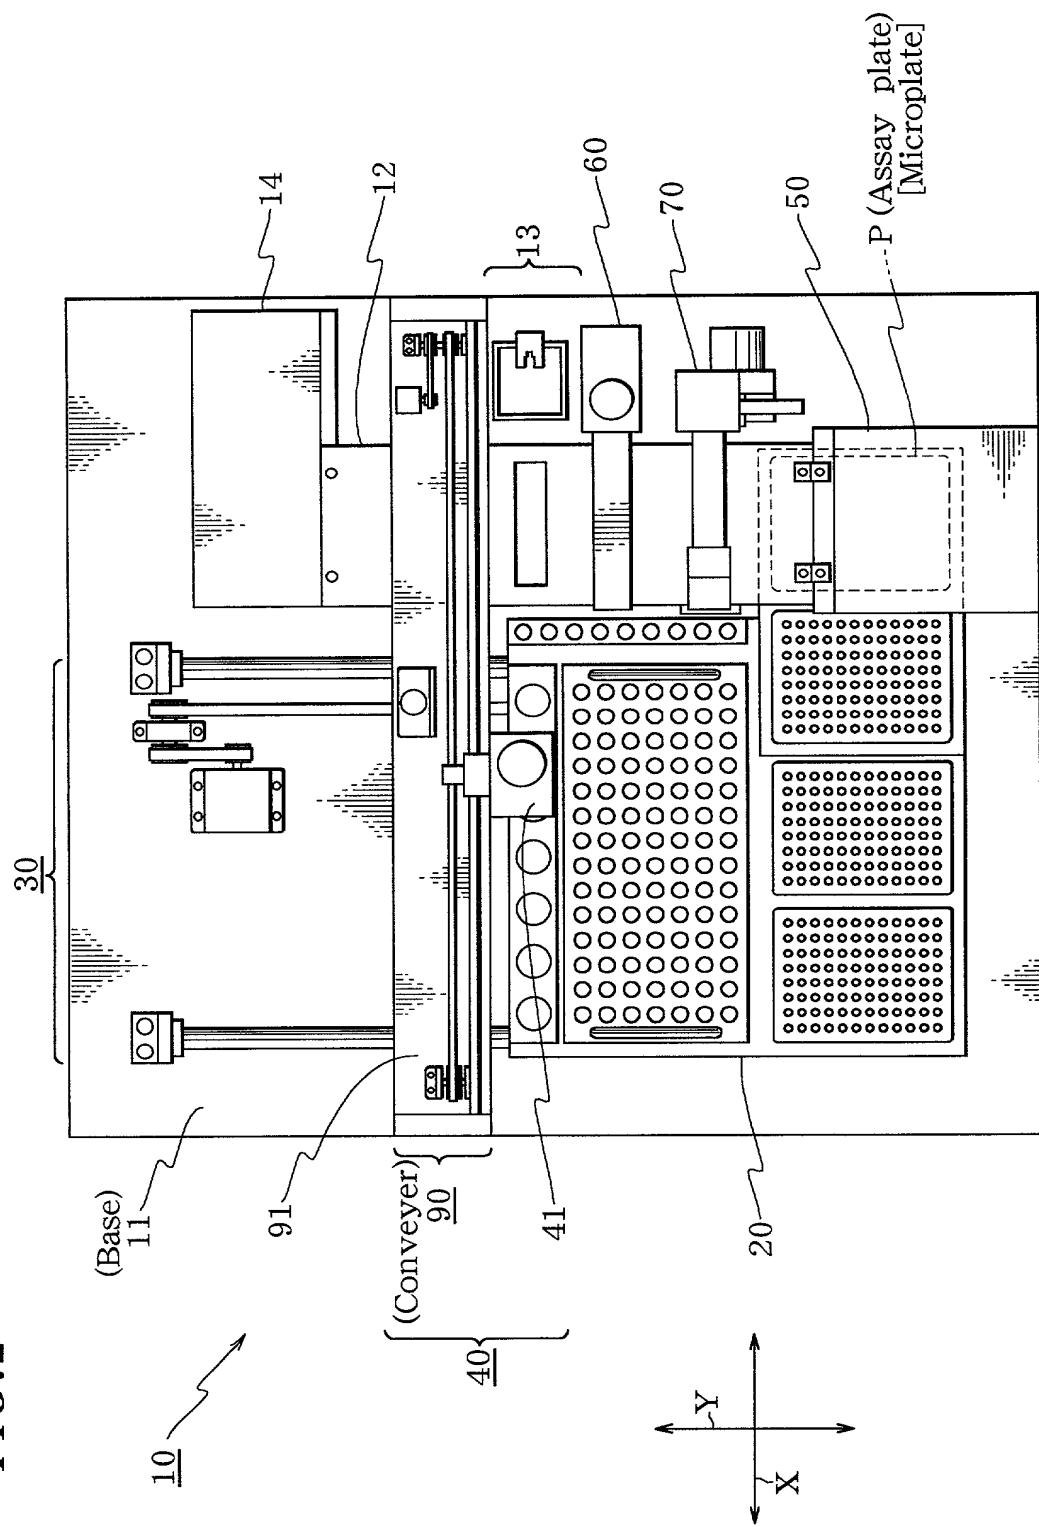

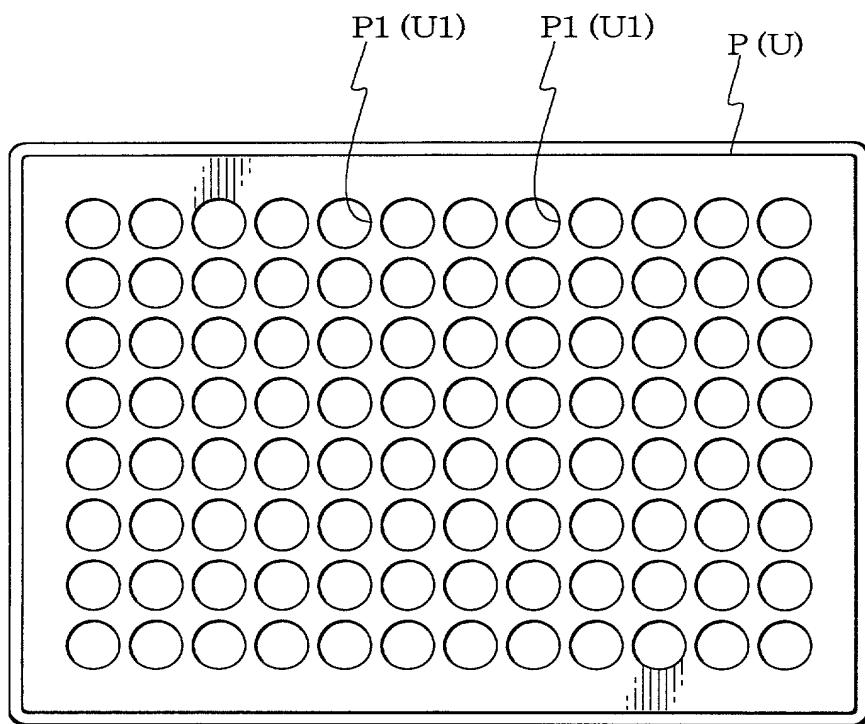
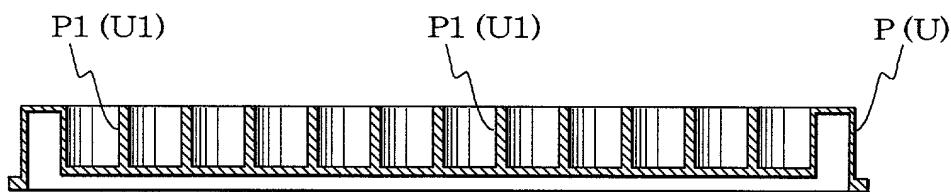
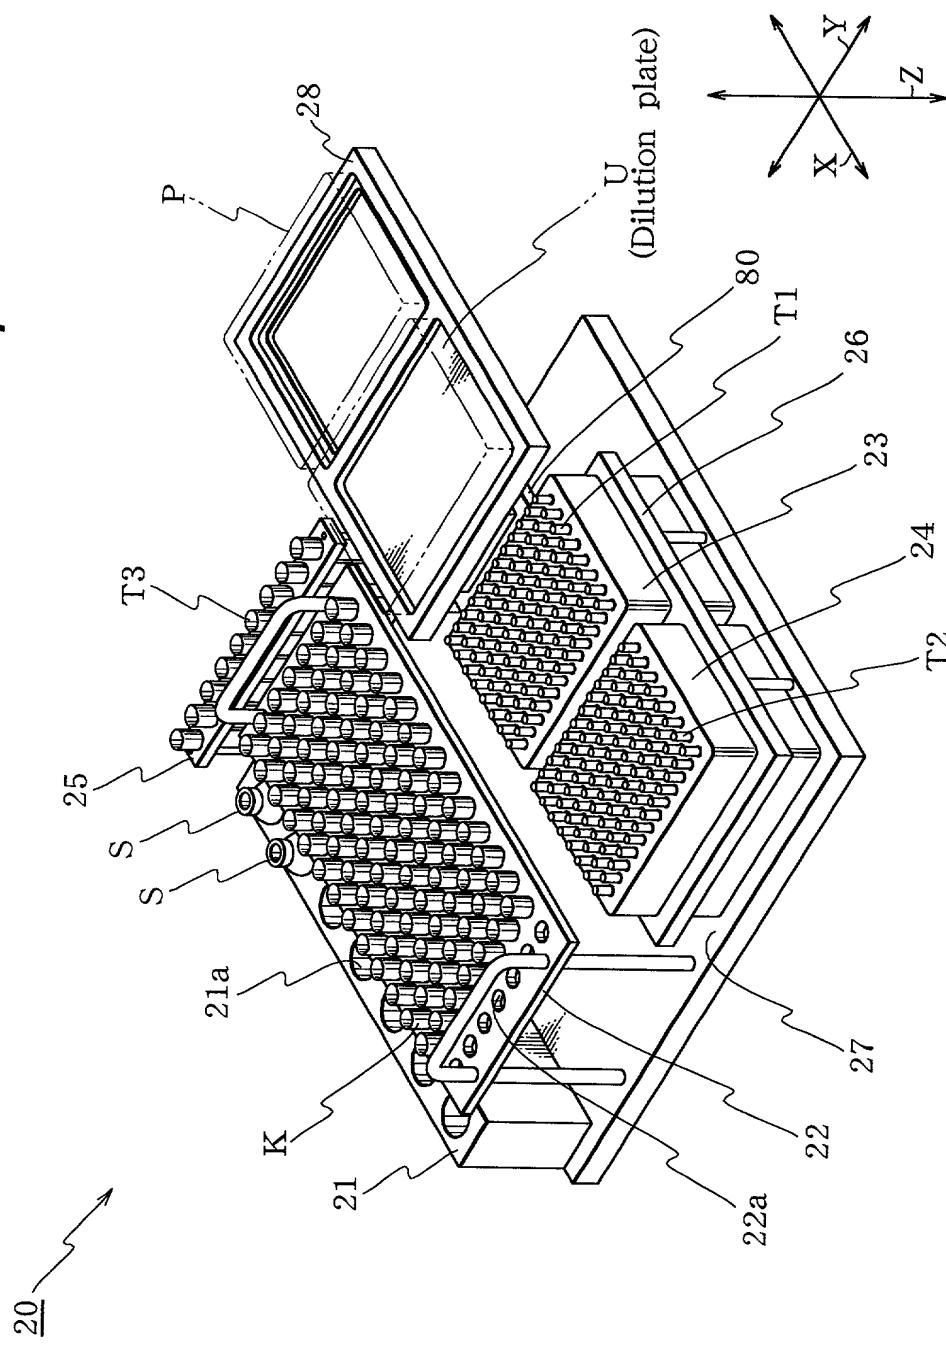
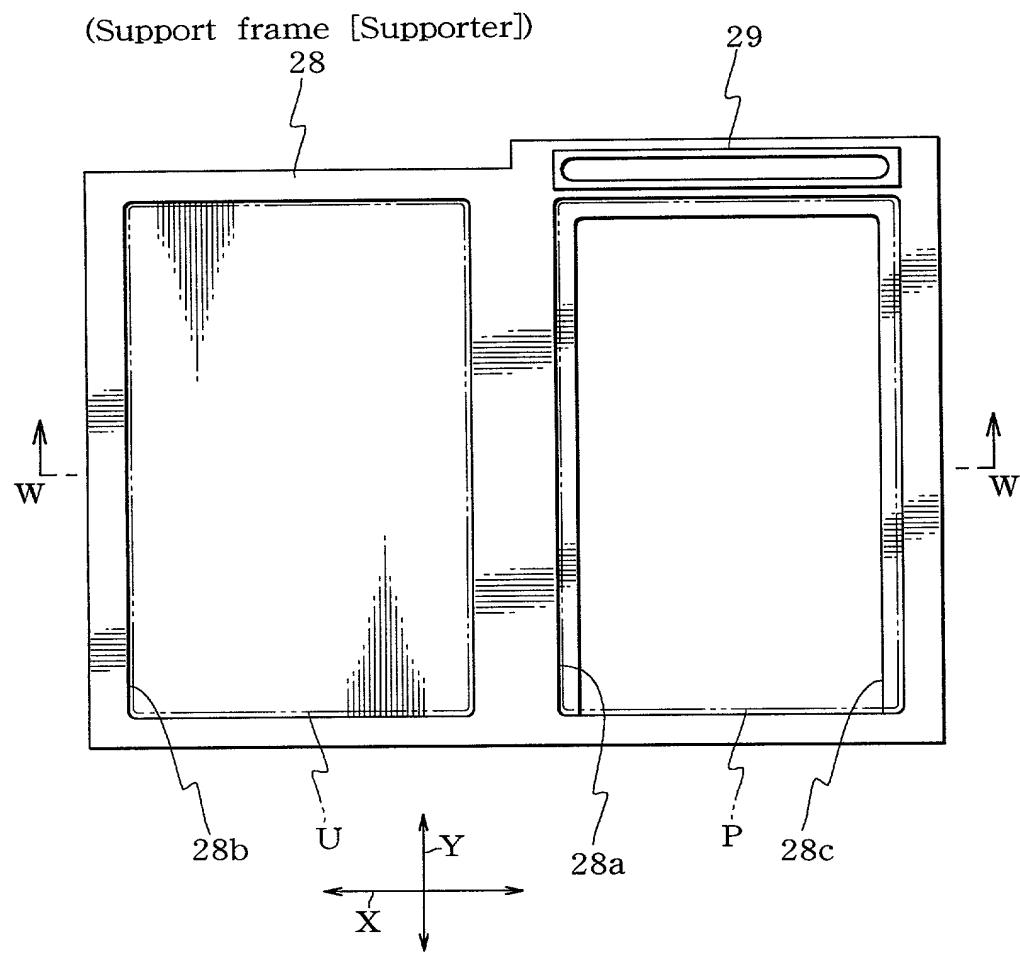
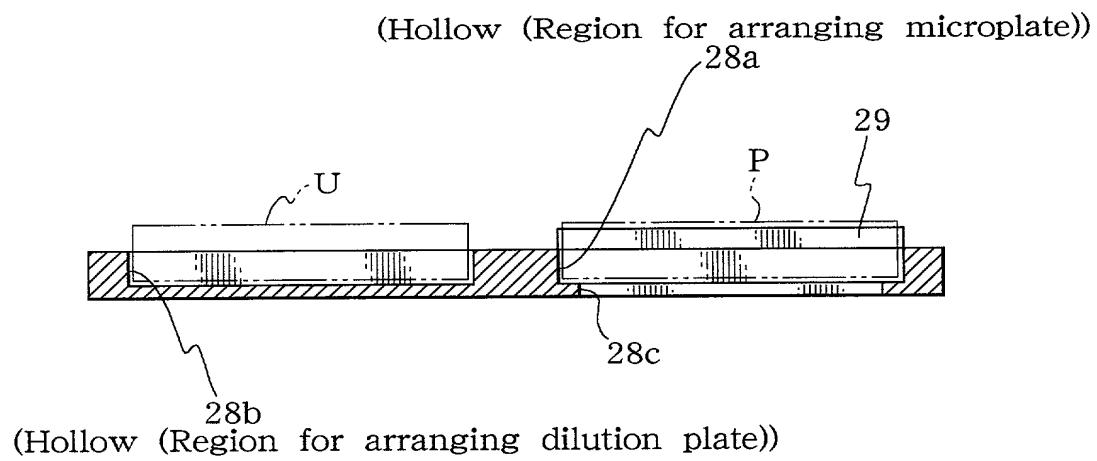
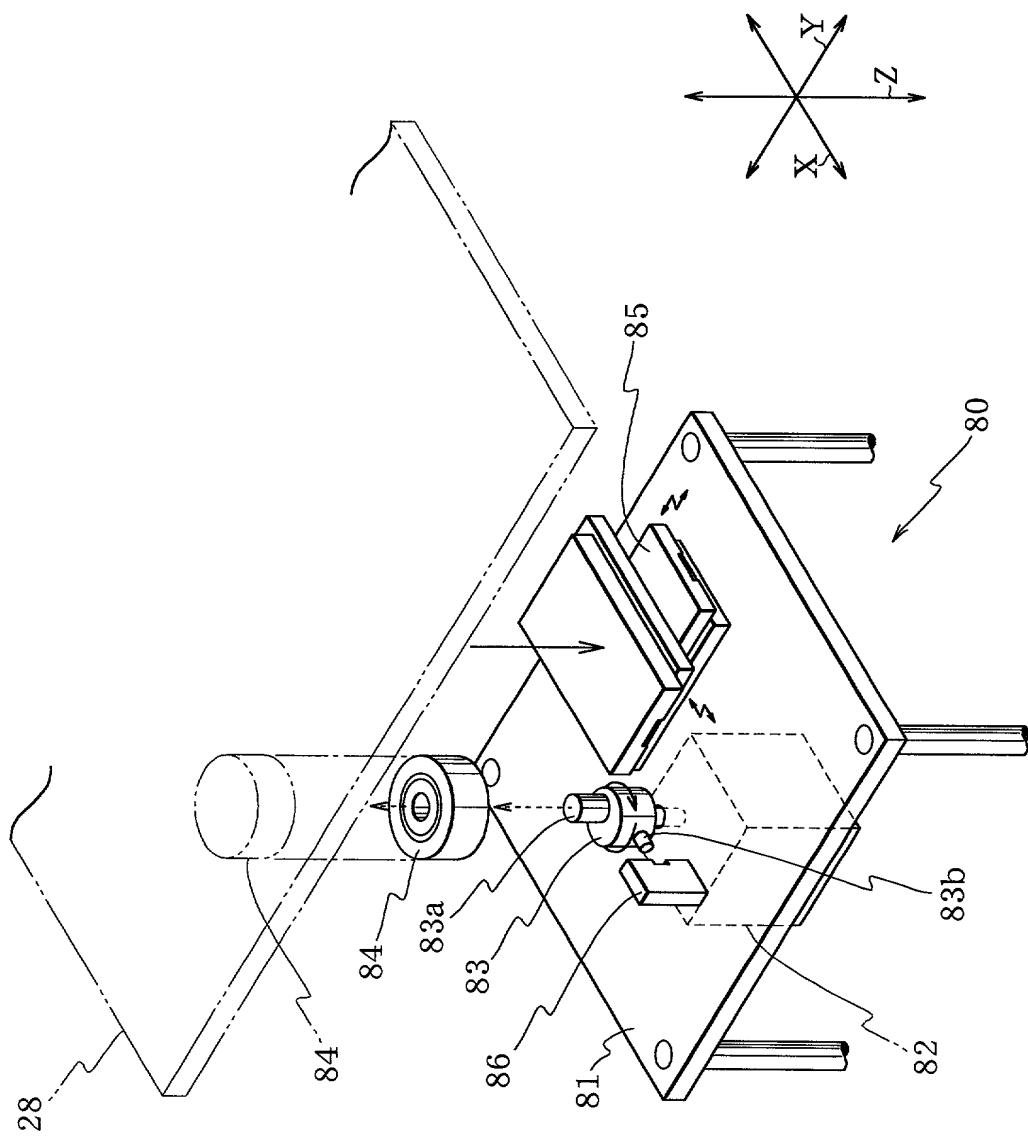
**FIG. 3(A)****FIG. 3(B)**

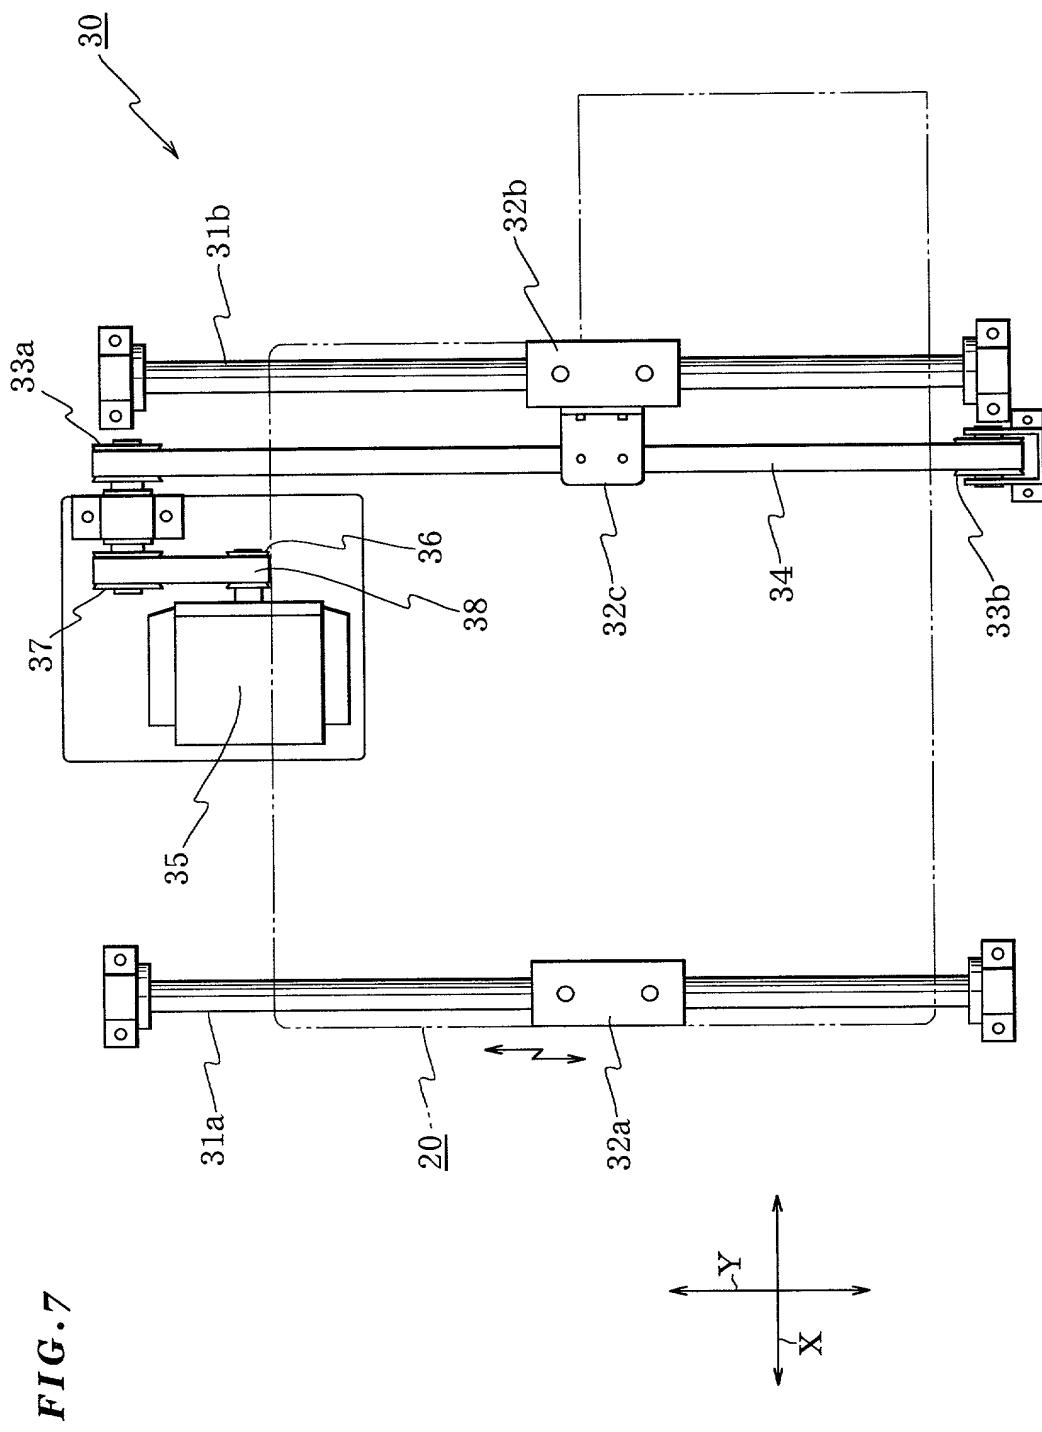
FIG. 4

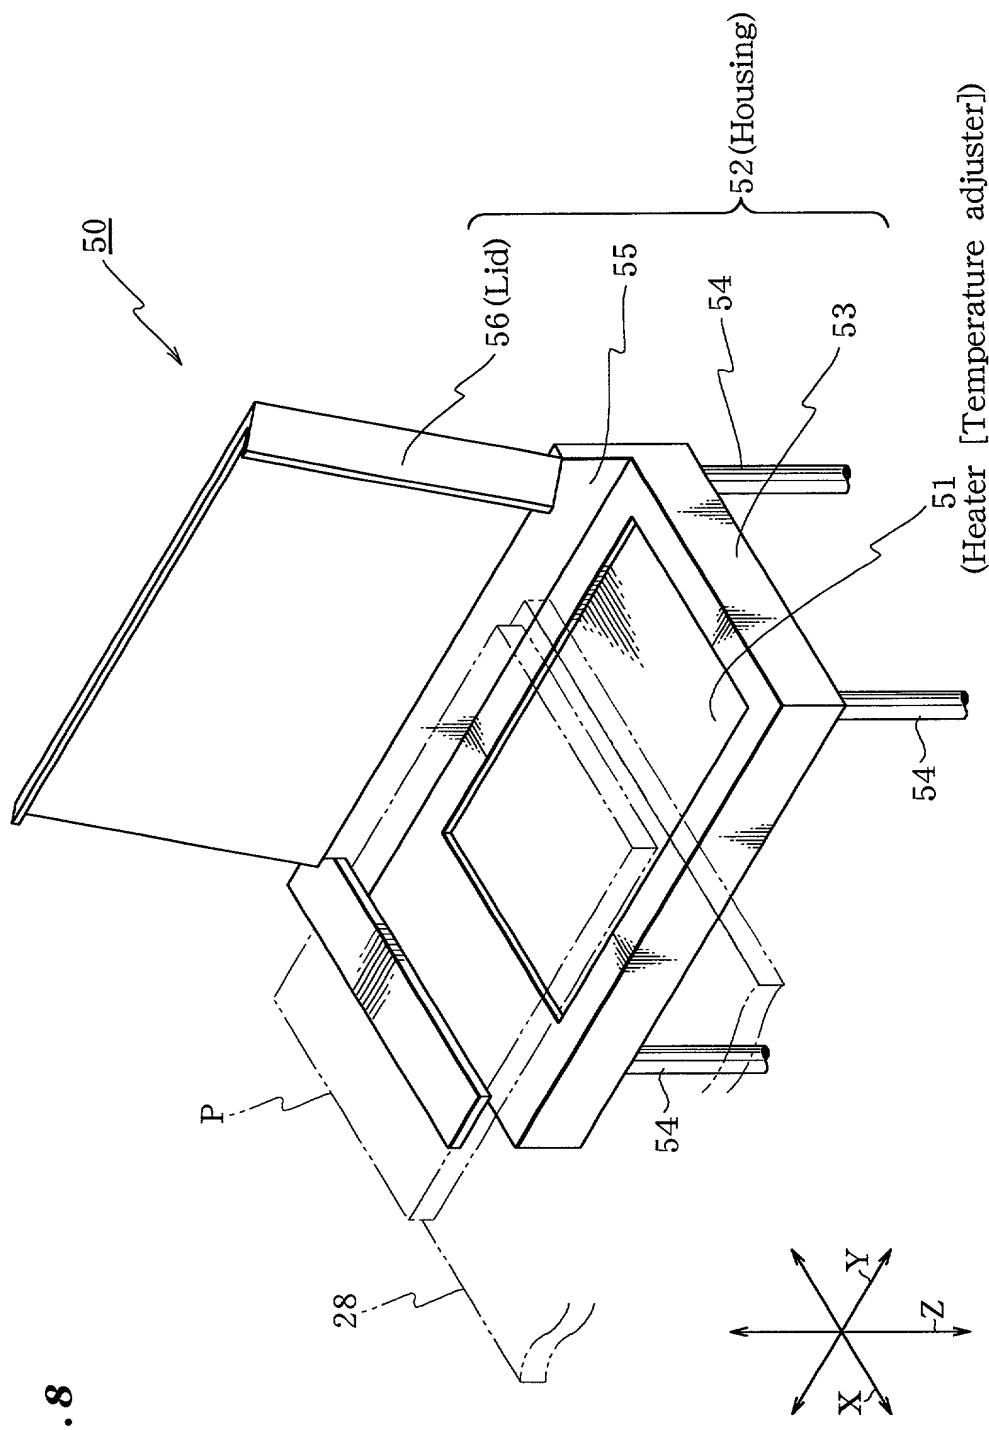



**FIG.5(A)****FIG.5(B)**



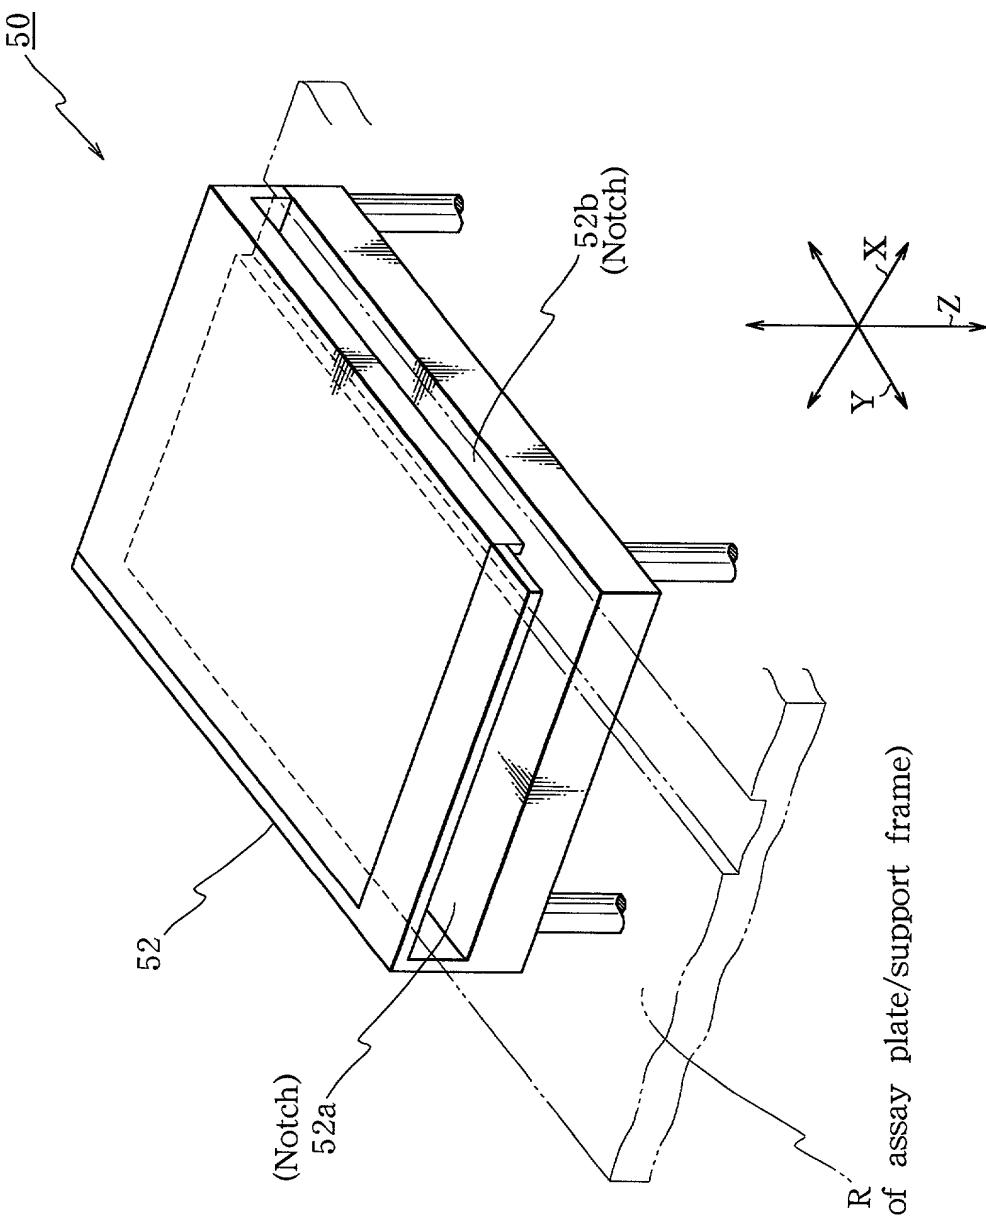**FIG. 6**







(Translation region of assay plate/support frame)


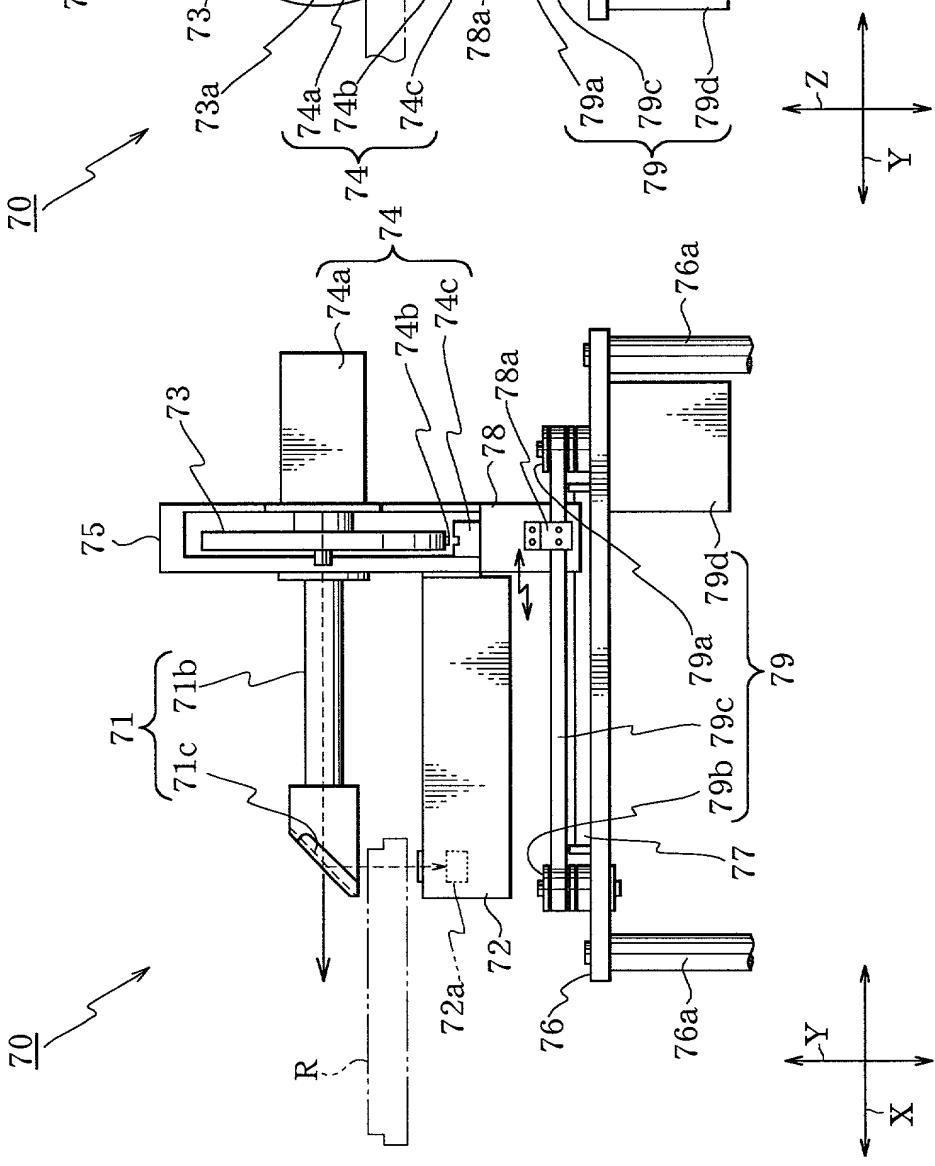
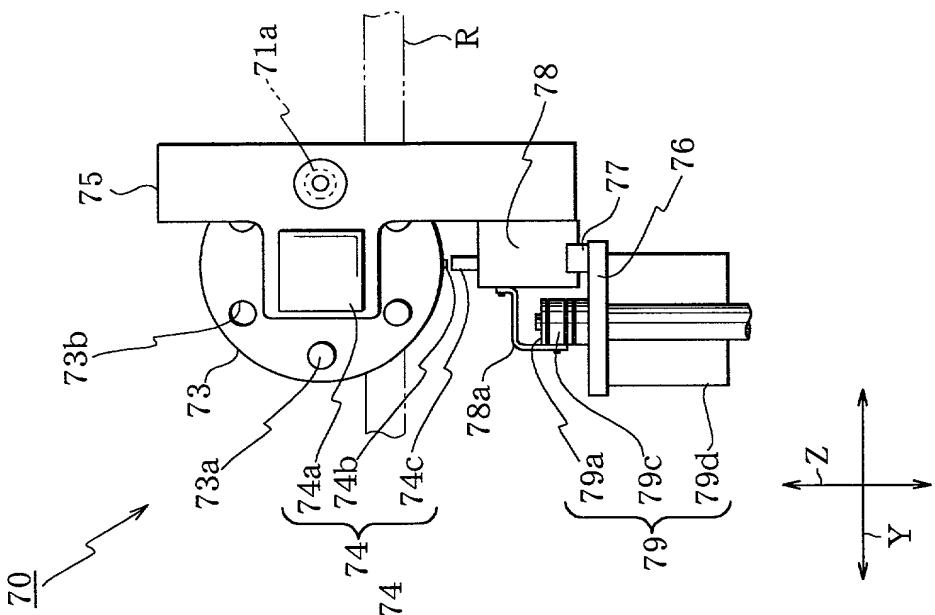
**FIG. 10 (A)****FIG. 10 (B)**

FIG. 11

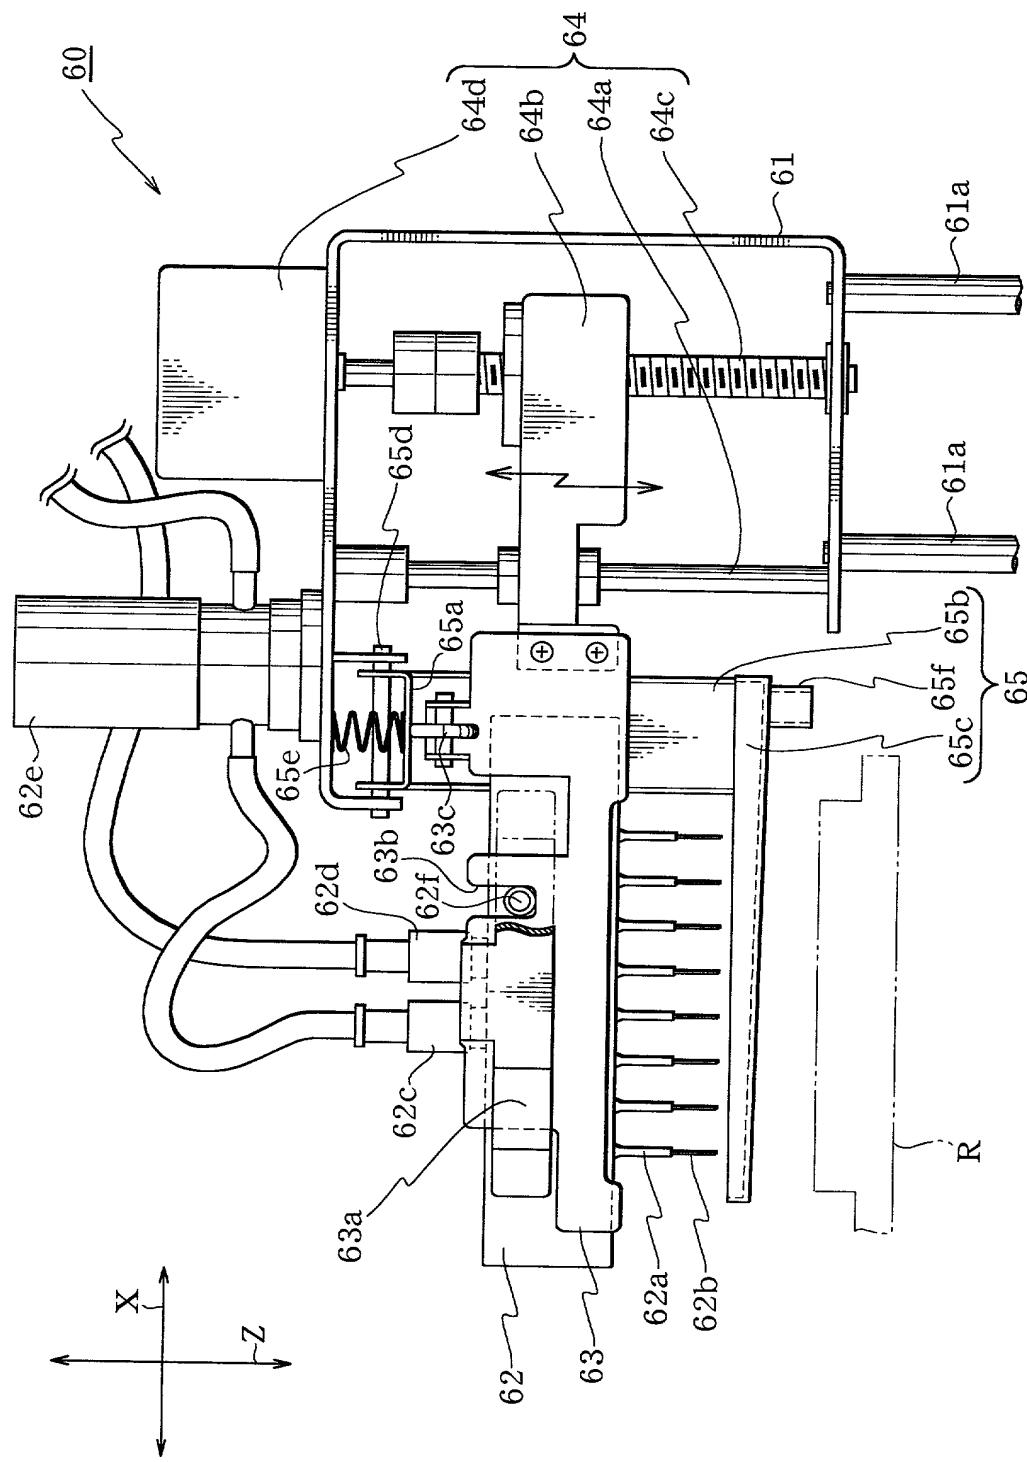

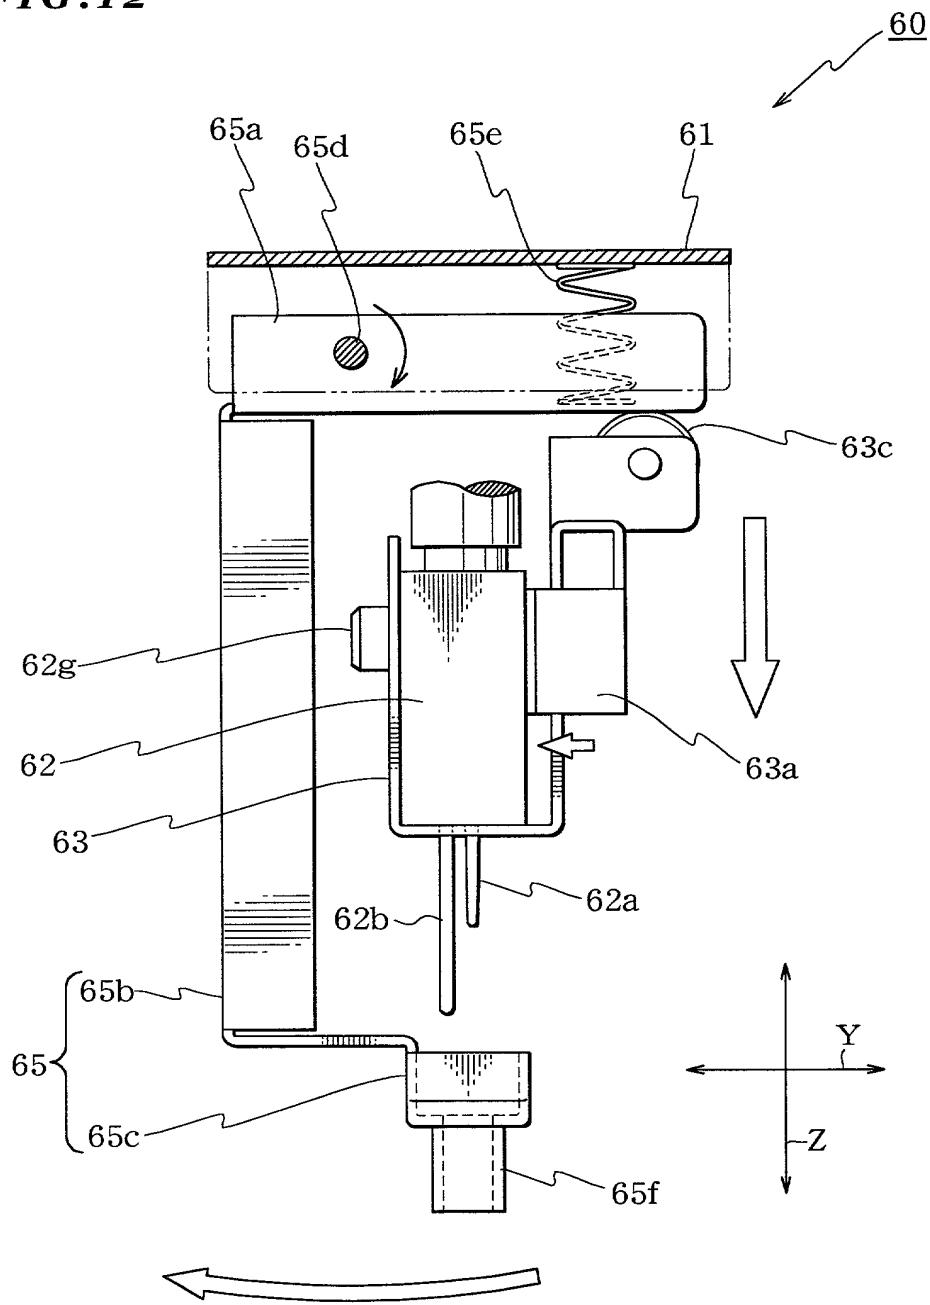
**FIG. 12**

FIG. 13



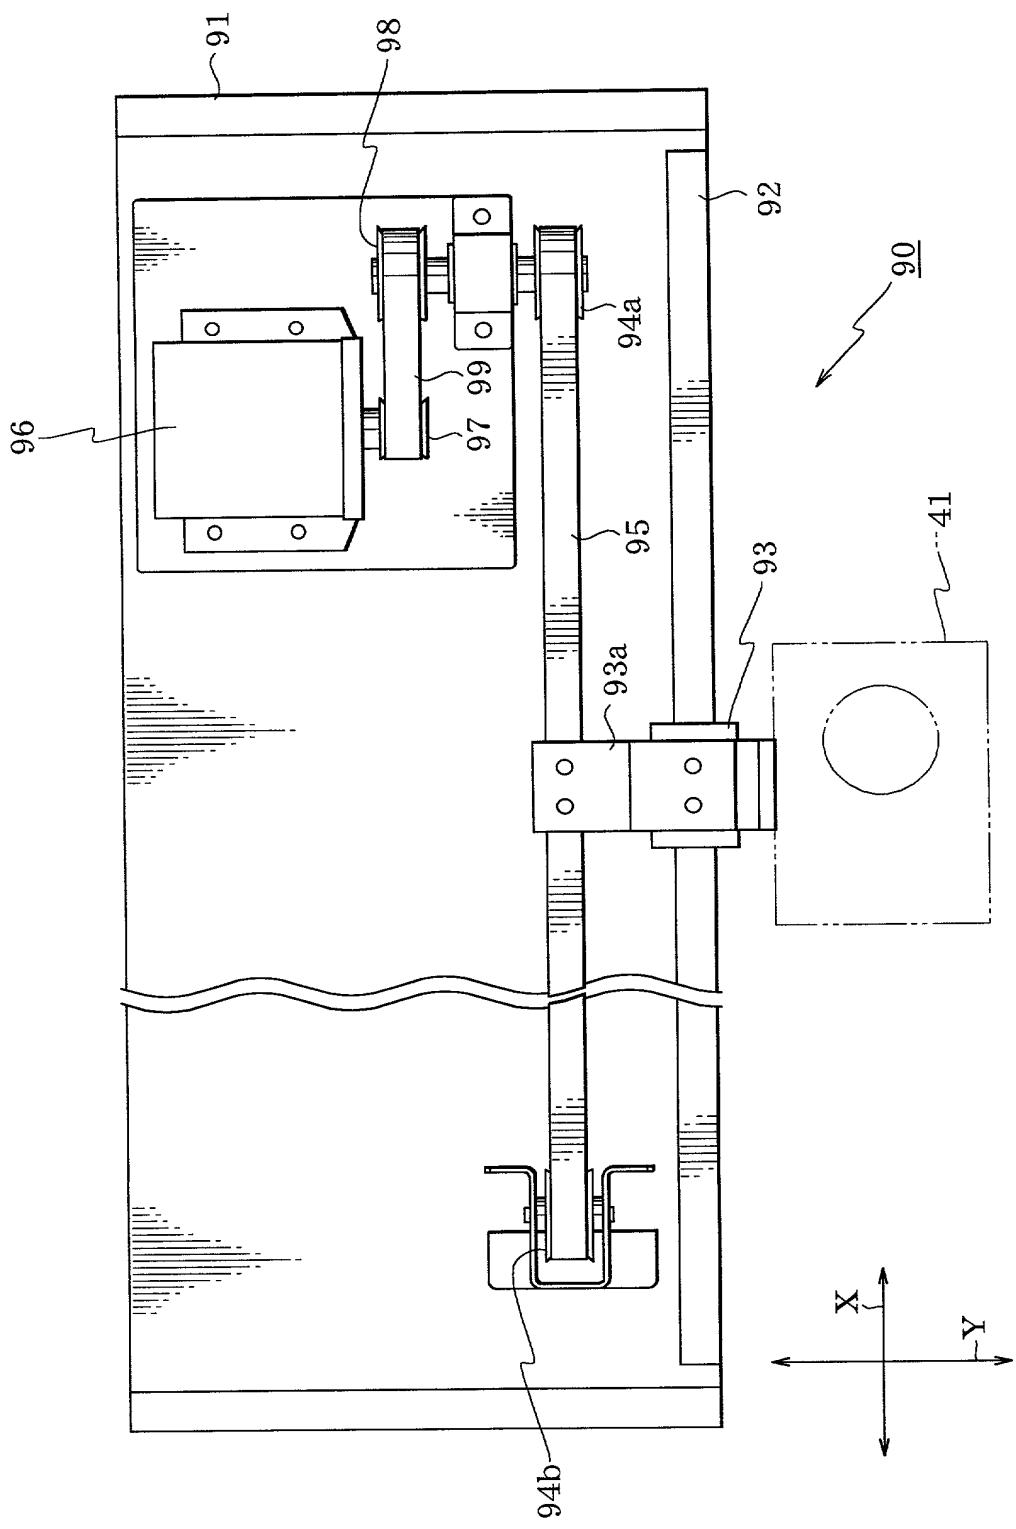



FIG. 14

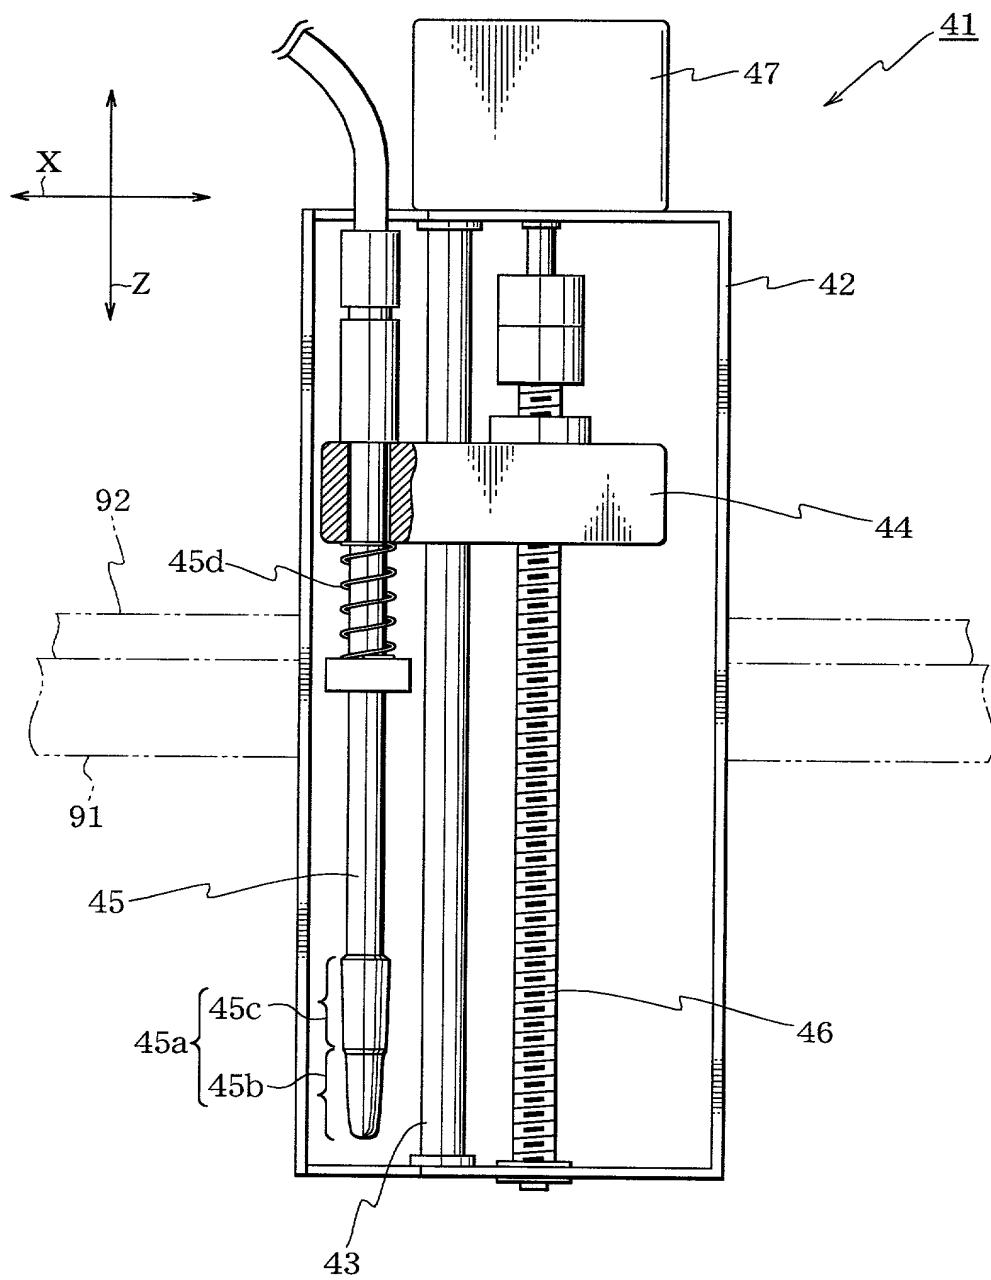

*FIG. 15 (A)*

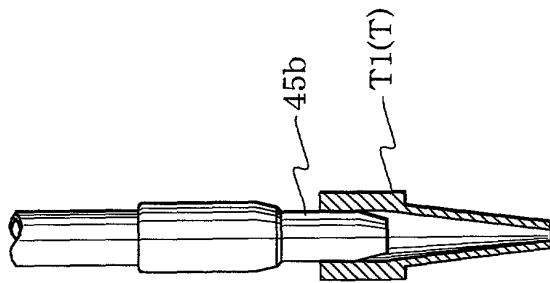

*FIG. 15 (B)*

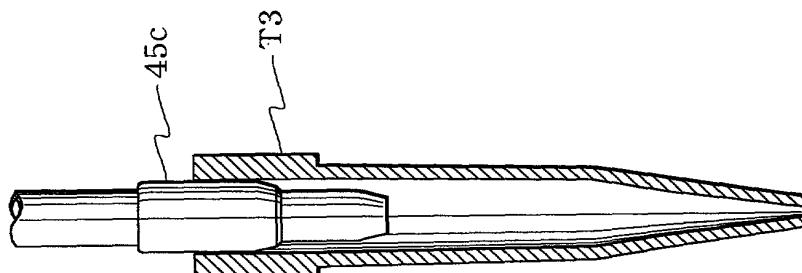

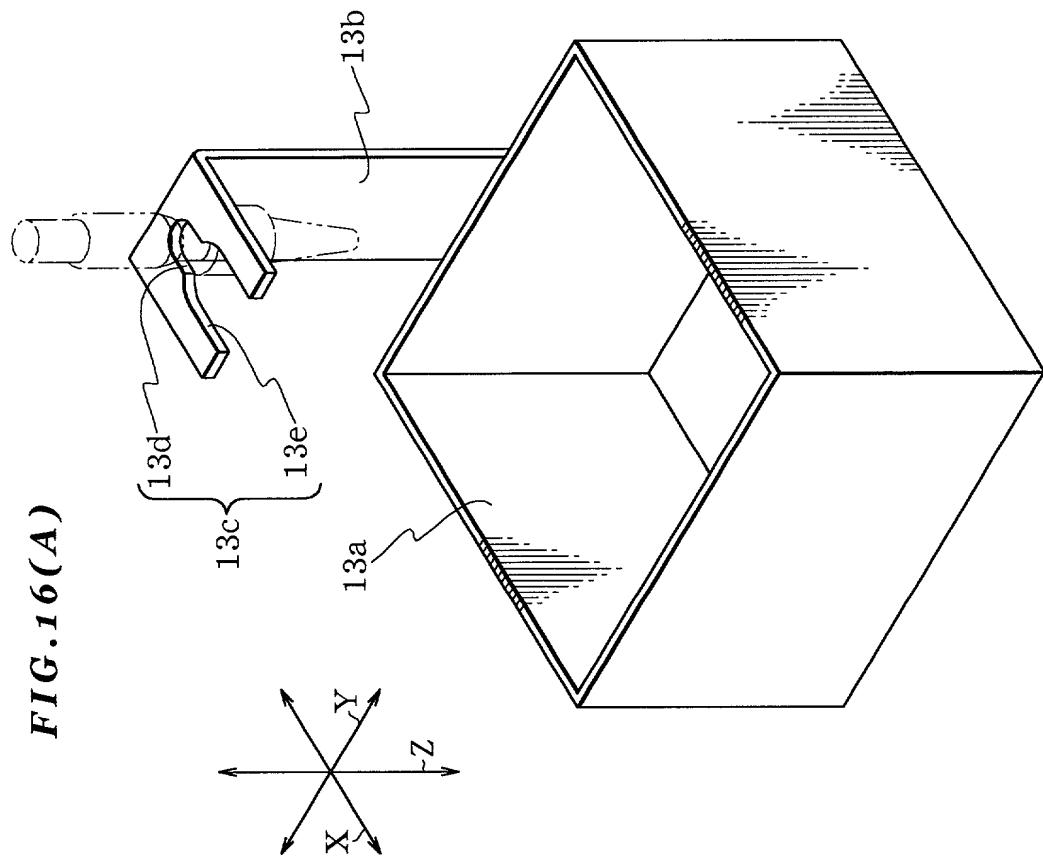
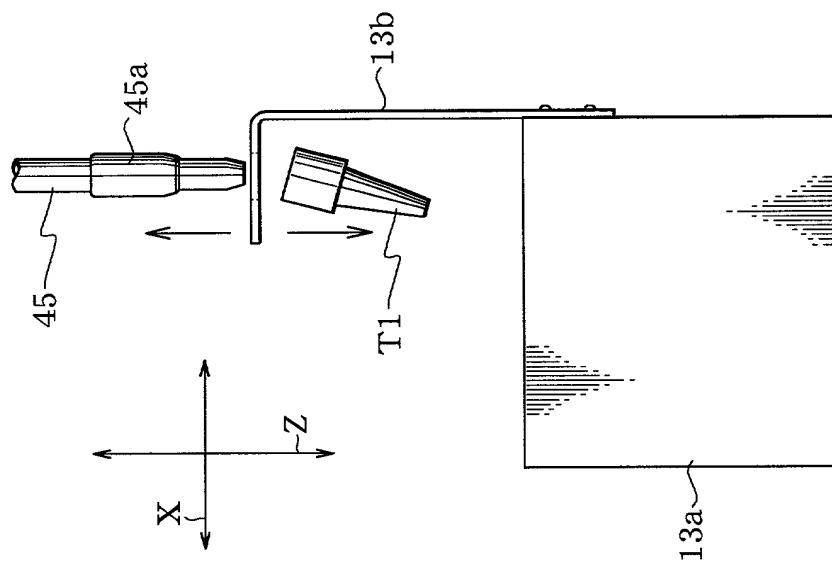
**FIG. 16(A)****FIG. 16(B)**

FIG. 17


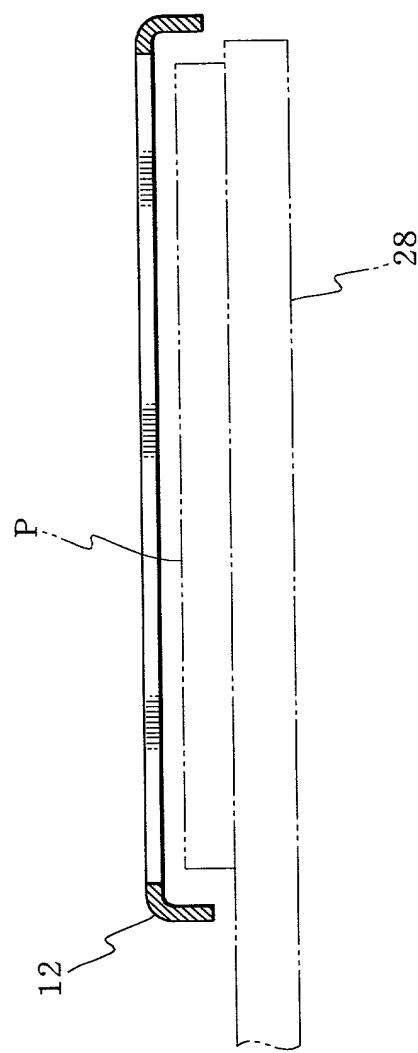


FIG. 18

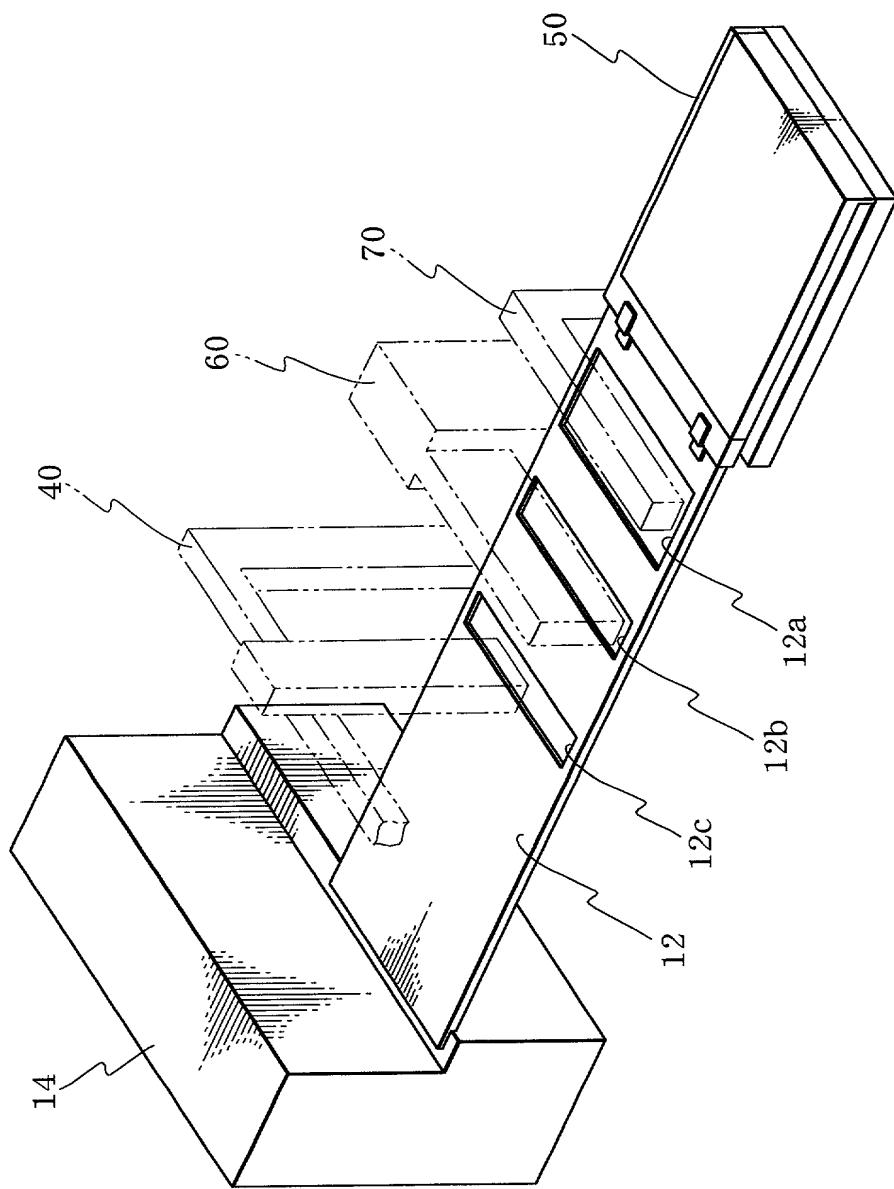

**FIG. 19**